


Rinse/Cleaner-A

GLOSSARY OF SYMBOLS

Symbols	Meaning of Symbols
	Consult instructions for use
	Date of manufacture
	Store at 15° C - 30° C.
	Expiry date
	Manufacturer
	Keep away from sunlight
	Lot number
	Keep dry
	<i>in-vitro</i> diagnostic medical device
	Handle with care
	Direction upward

Rinse/Cleaner-A

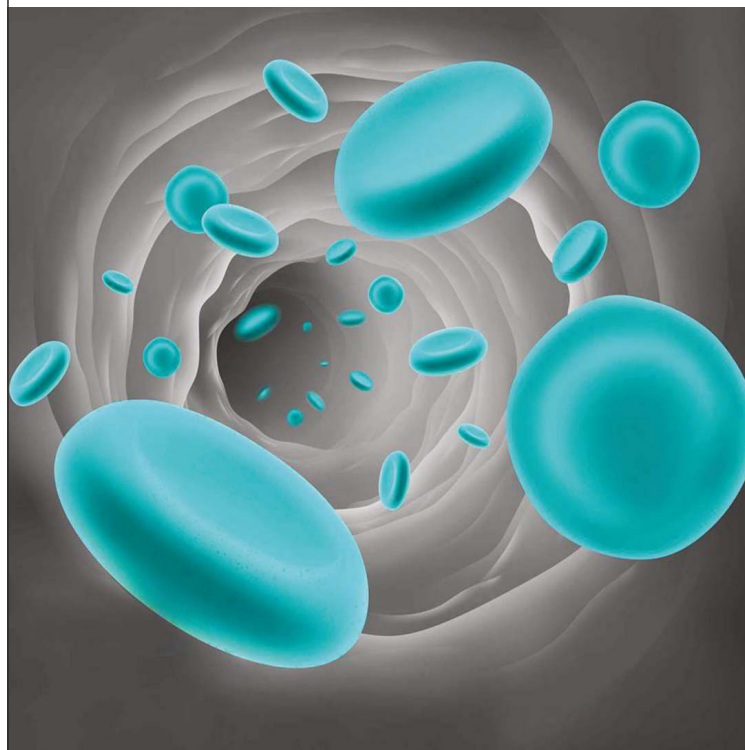

Manufactured by:

VANGUARD DIAGNOSTICS (P) LIMITED

C-123, Phase-I, Okhla Industrial Area,
New Delhi- 110 020, India.



011-41727222



info@vanguarddiagnostics.com



www.vanguarddiagnostics.com

PM300091170



Rinse/Cleaner-A

Pack Size : 1x 1 L



For *in-vitro* use only. Not for medicinal use.

Rinse/Cleaner-A

INTENDED USE

Cleaner-A is used for cleaning the bath and tubing in Horiba ABX 3-Part differential Hematology Analyzers.

Please refer to the analyzer's User Manual for further information.

ACTIVE INGREDIENTS

Sodium Chloride	: 1.2%
Triton- X 405	: 0.2%
Proteolytic Enzymes	: 1.1%
MonoPhenyl Glycol	: 0.5%
Preservative	: 0.01%

DIRECTIONS FOR USE



- 1) Personnel installing the reagent, should be a trained laboratory professional.
- 2) Open the bottle cap and connect it with the corresponding Cleaner-A tubing as per the instructions given in the analyzer's User Manual.
- 3) Avoid contamination of the tubing and the reagent.
- 4) Do not pour and mix the remains of a reagent from a container, into another one.
- 5) Prime thoroughly with the new reagent and measure background values according to the analyzer's User Manual.
- 6) When installing a new lot of the reagent, recalibrate the instrument as specified in the User Manual.

Rinse/Cleaner-A

PRECAUTIONS

	Rinse/Cleaner-A, is for in-vitro diagnostics use only.
	Rinse/Cleaner-A is environmental friendly and does not contain harmful ingredients.
	Do not inhale the reagent or pipette by mouth.
	Avoid contact with skin/eyes. In case of contact, wash off immediately with plenty of water and seek medical attention, as early as possible.
	Do not use if package is damaged.
	Keep the reagent container closed when not in use.
	Wear protective gloves when handling the reagent.
	Please refer to the MSDS associated with the reagent.
	Use Good Laboratory Practices (GLP) when handling the reagent.

Rinse/Cleaner-A

SPECIMEN COLLECTION AND STORAGE

Blood specimens should be collected by vein puncture in EDTA anticoagulant.

Specimens for hematological analysis may be stored at 15°- 30°C for 2 - 4 hours or at 2°- 8°C for 24 hours after collection.

REAGENT PREPARATION

This reagent is ready for use and can be connected to the analyzer directly from the container; no special reagent preparation is required.

STORAGE, STABILITY AND DISPOSAL

- Store Cleaner-A between 15°and 30°C.
- The unopened reagent is stable up to the expiry date mentioned on the label when stored between 15°C - 30°C.
- Use Diluent within 06 months of first opening.
- Do not use reagent beyond the expiry date printed on the container label.
- Discard opened container after 06 months.
- Do not use reagent once frozen.
- Dispose waste product in accordance with local Government regulations.